

Figure 1

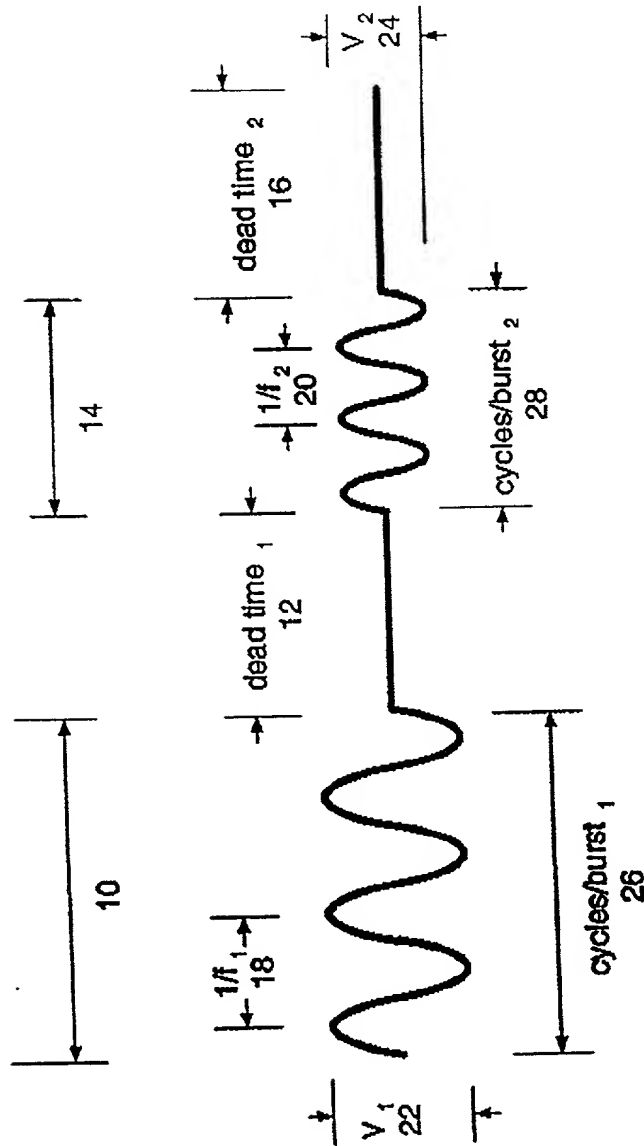


Figure 2






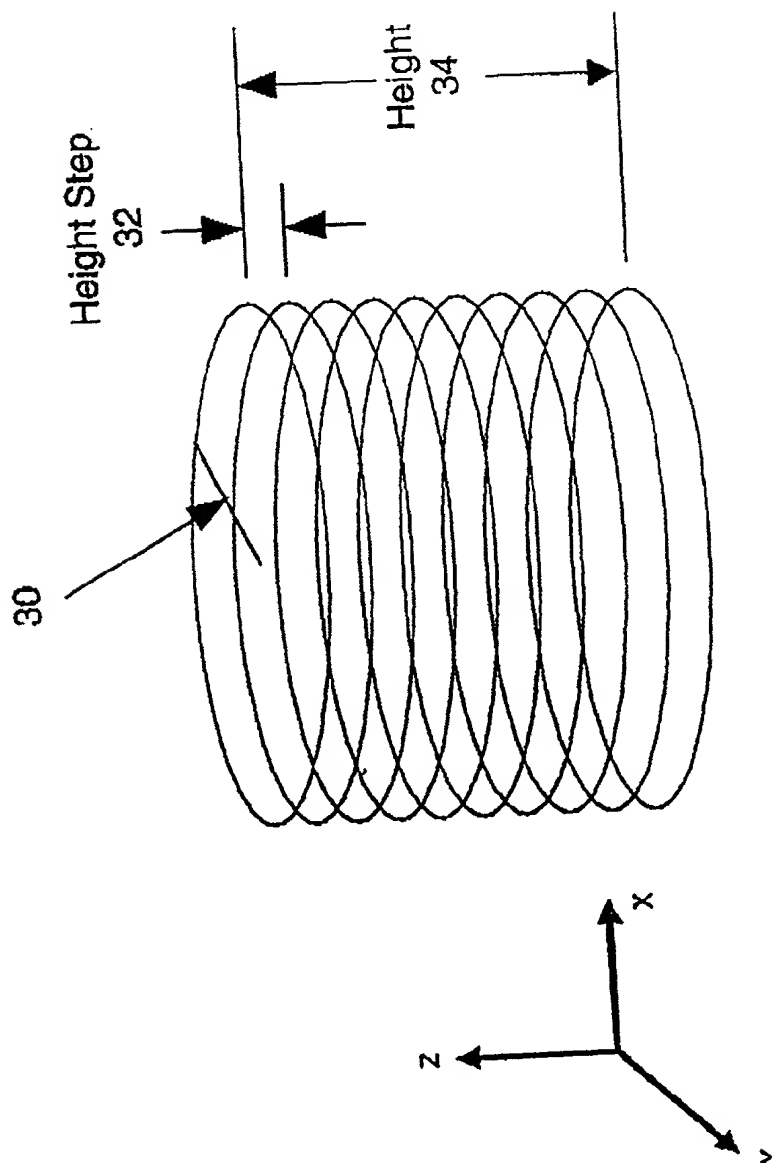


Figure 3




post-treatment transfer

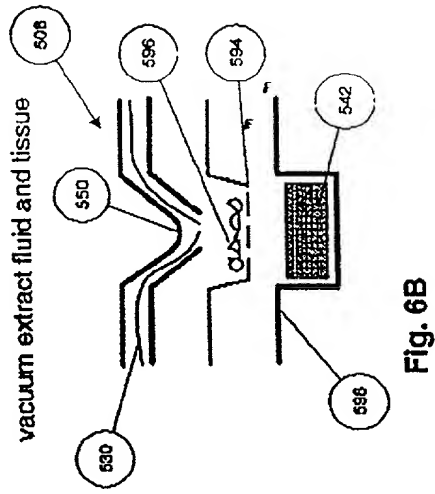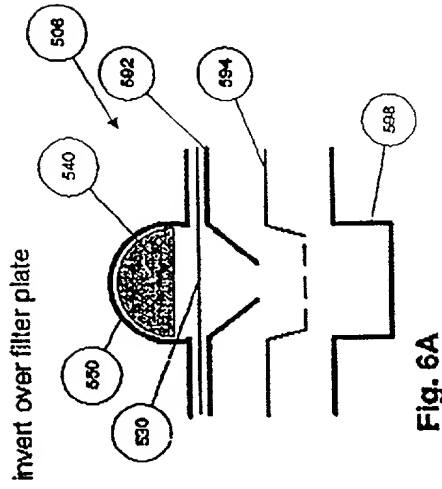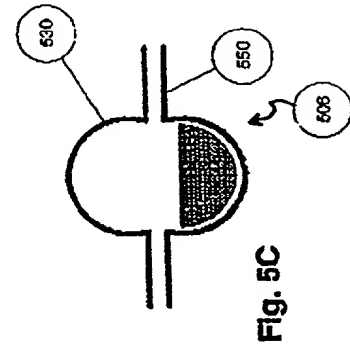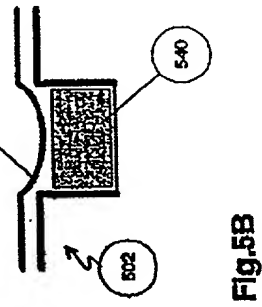

pre-treatment assembly

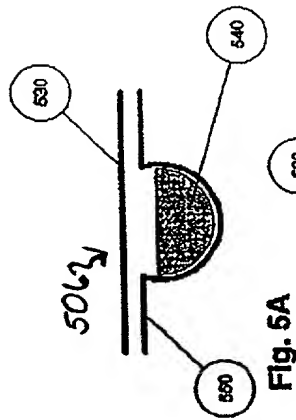

treatment vessels

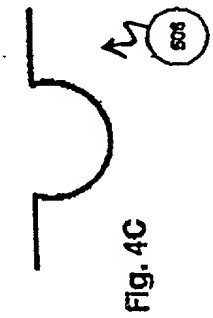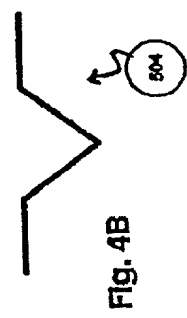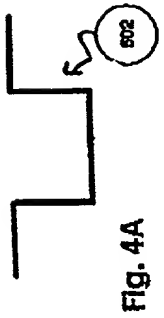

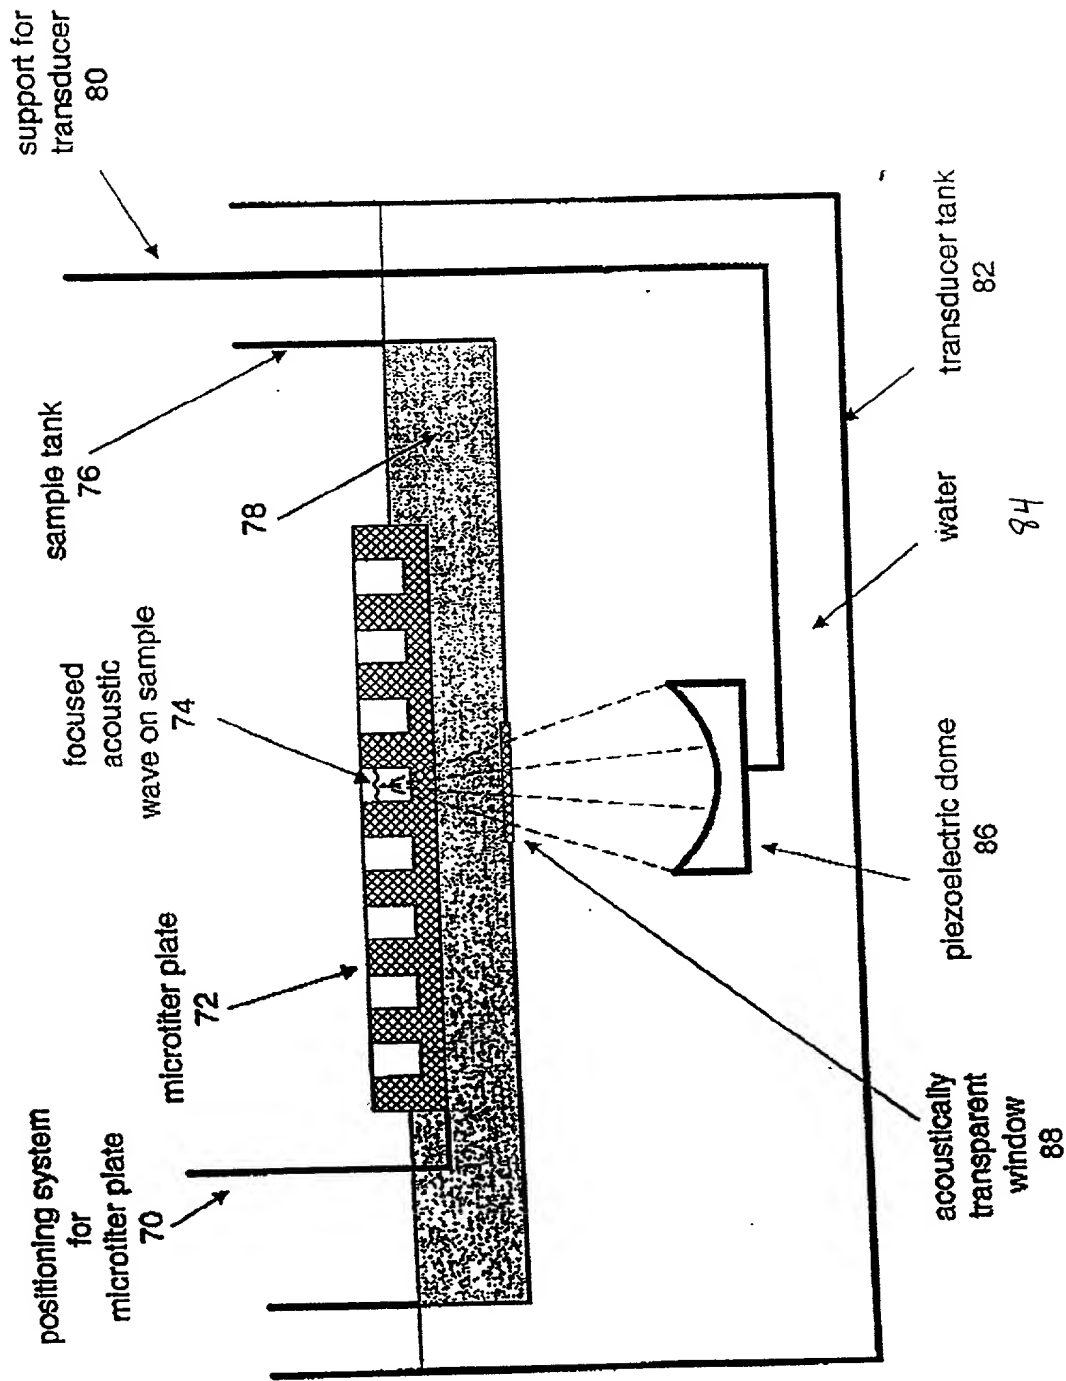


Figure 7



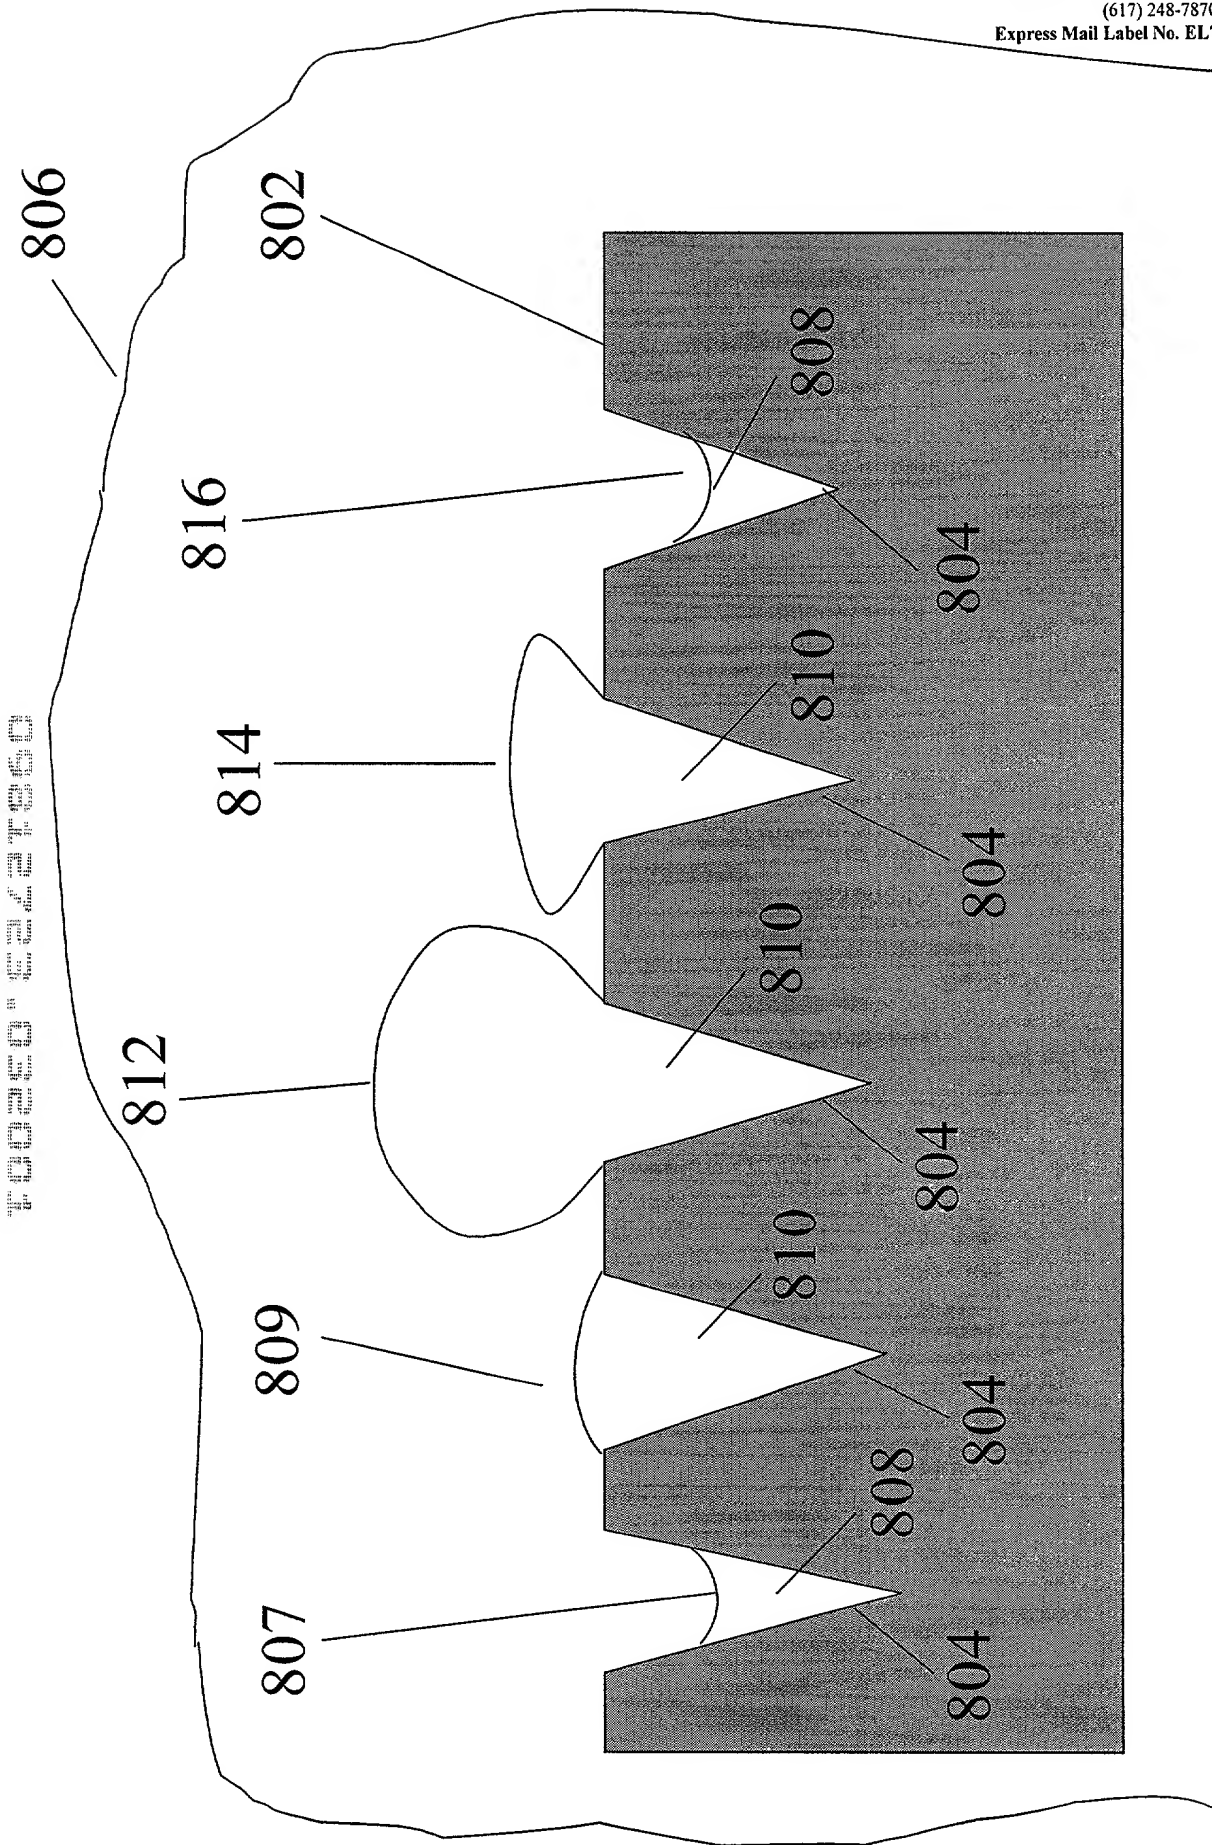


Figure 8
2046645

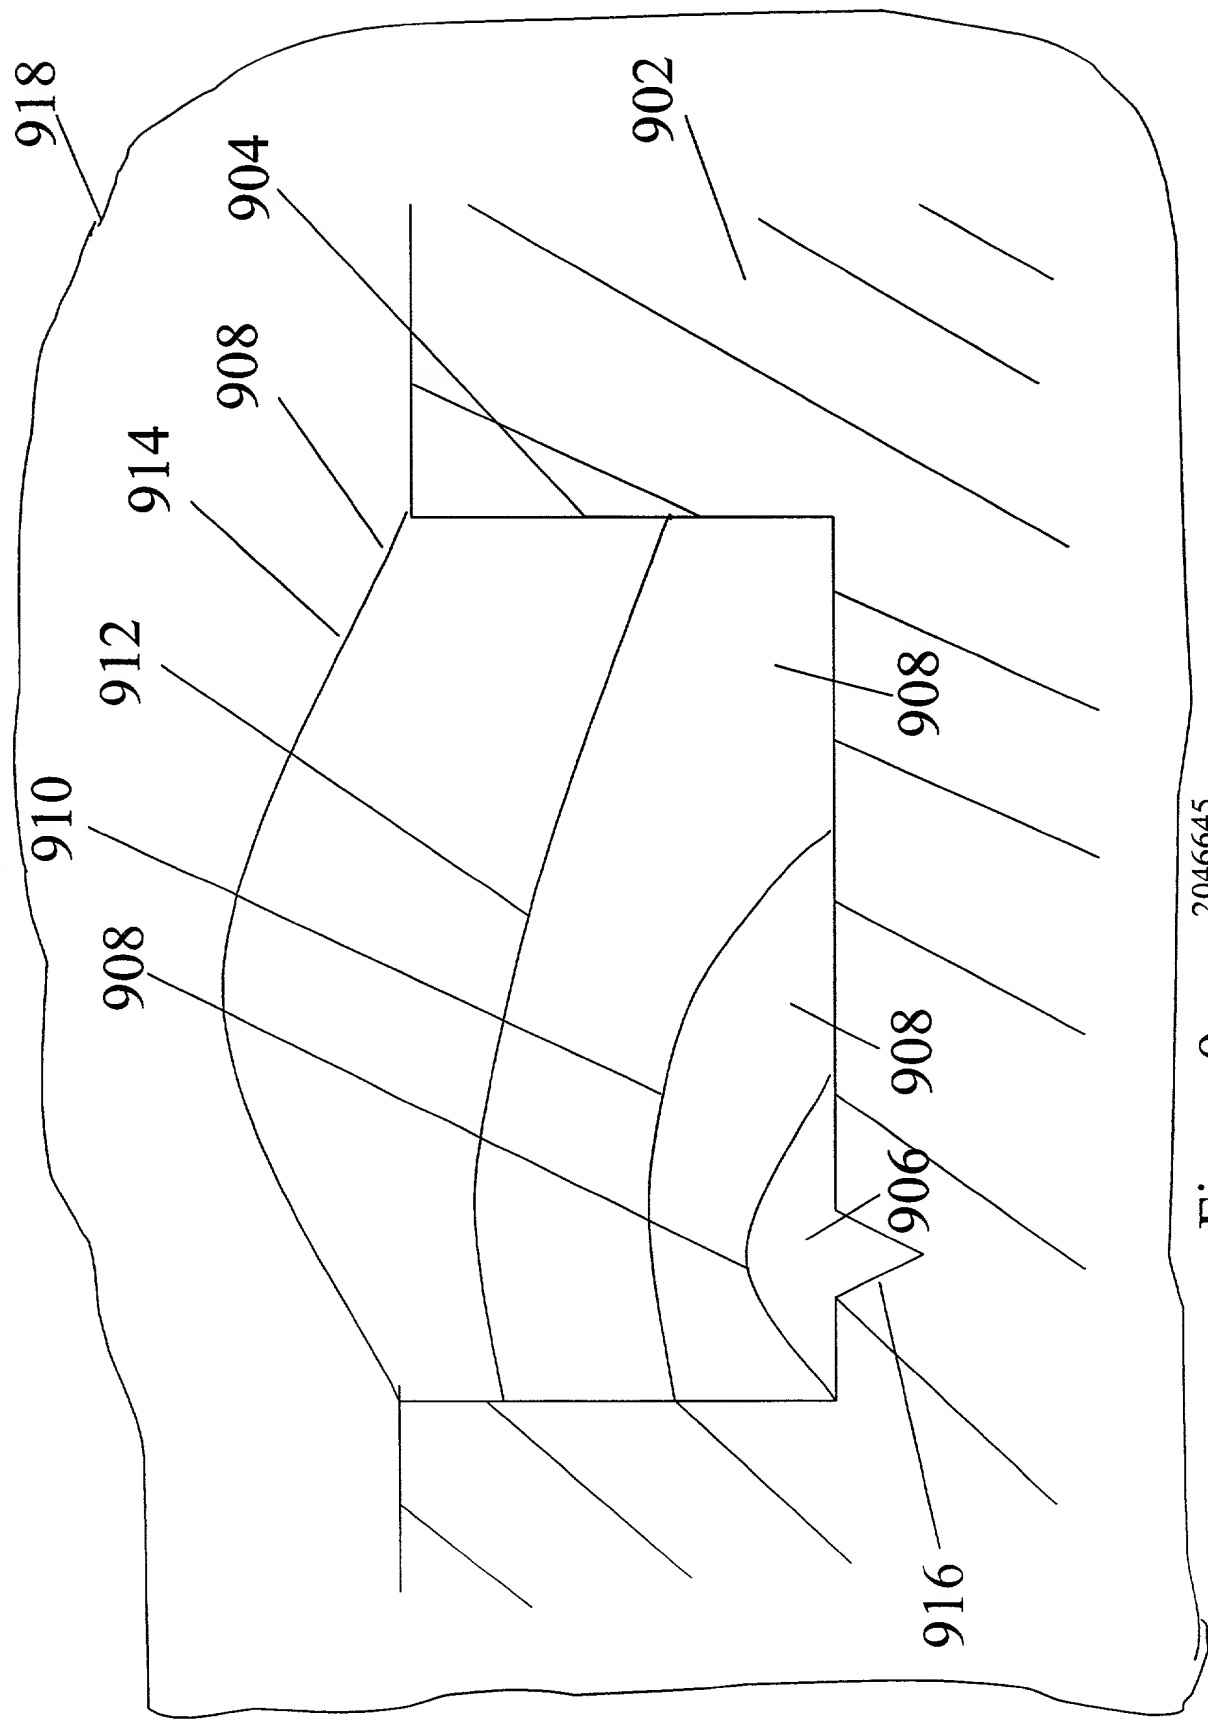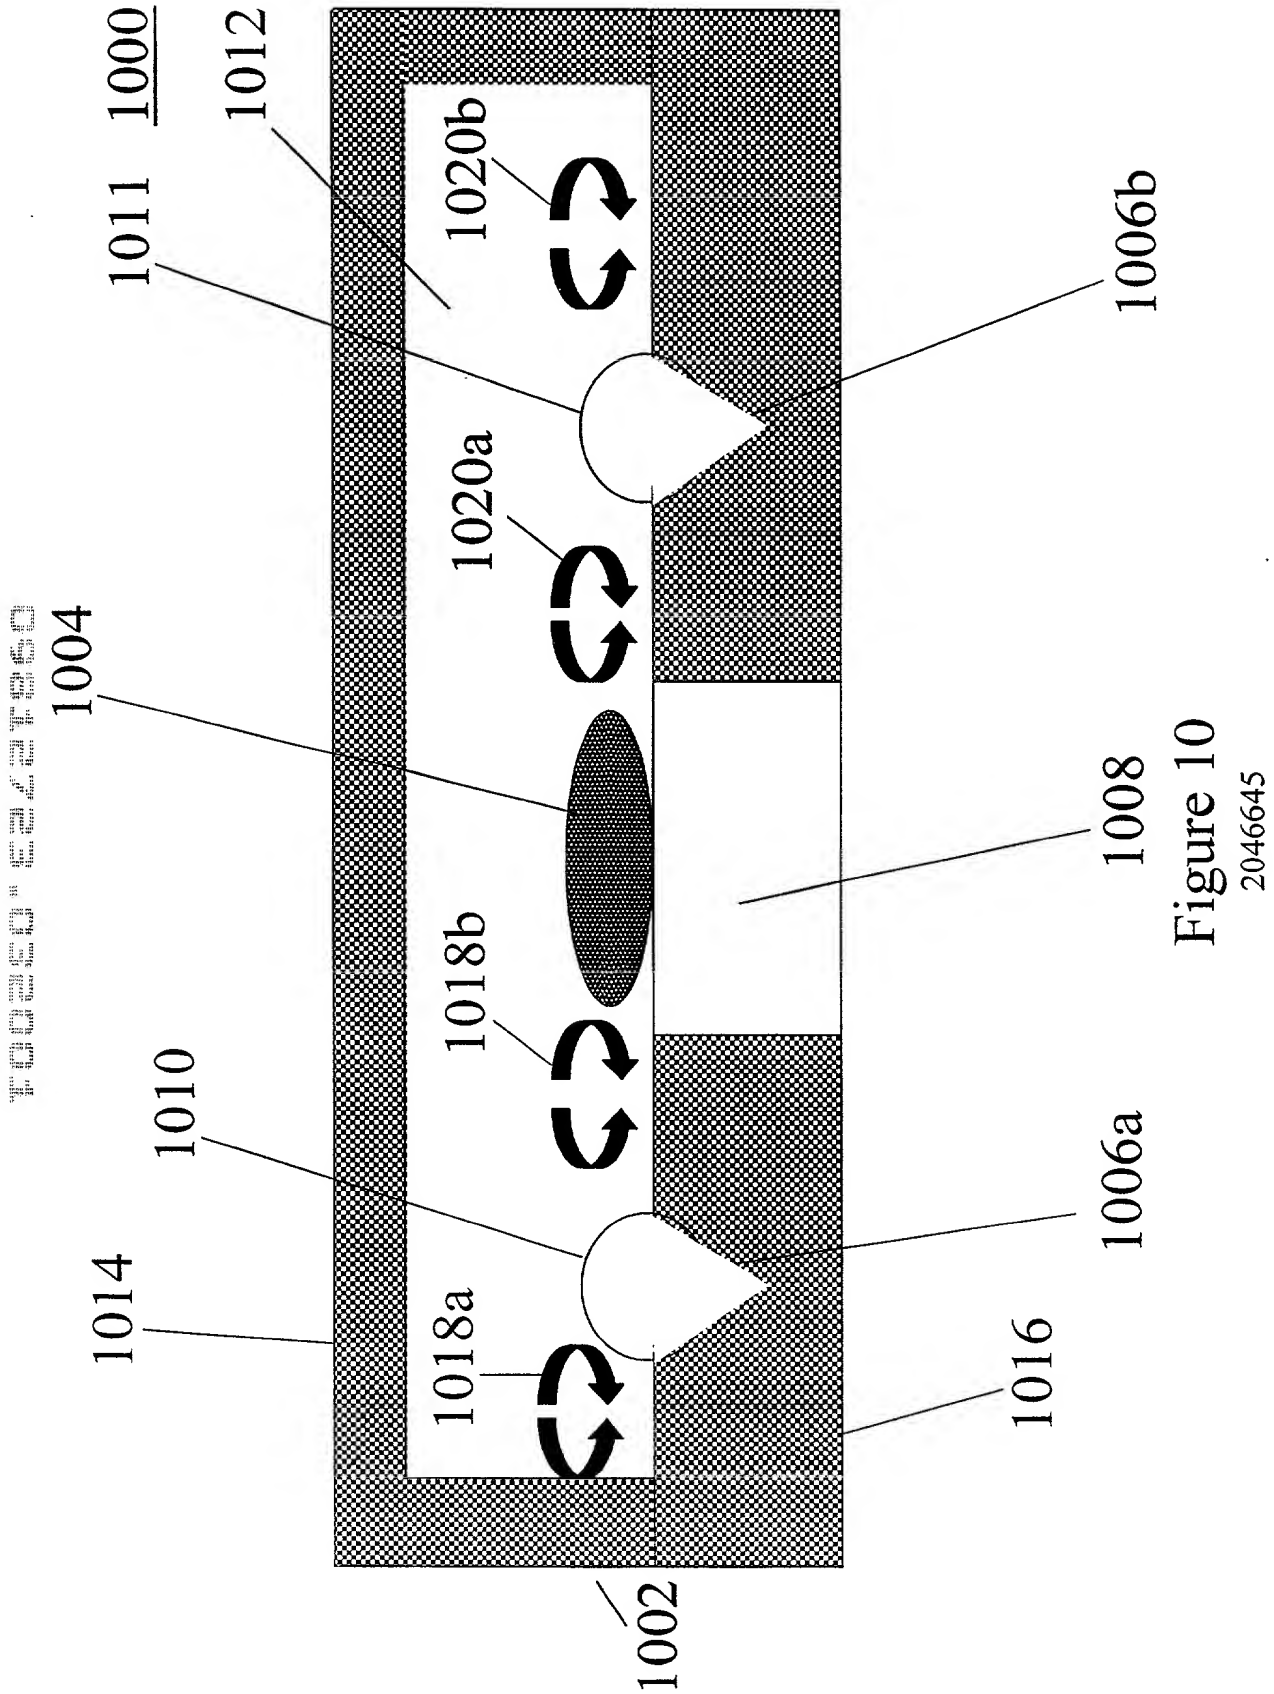

2046645

Figure 9



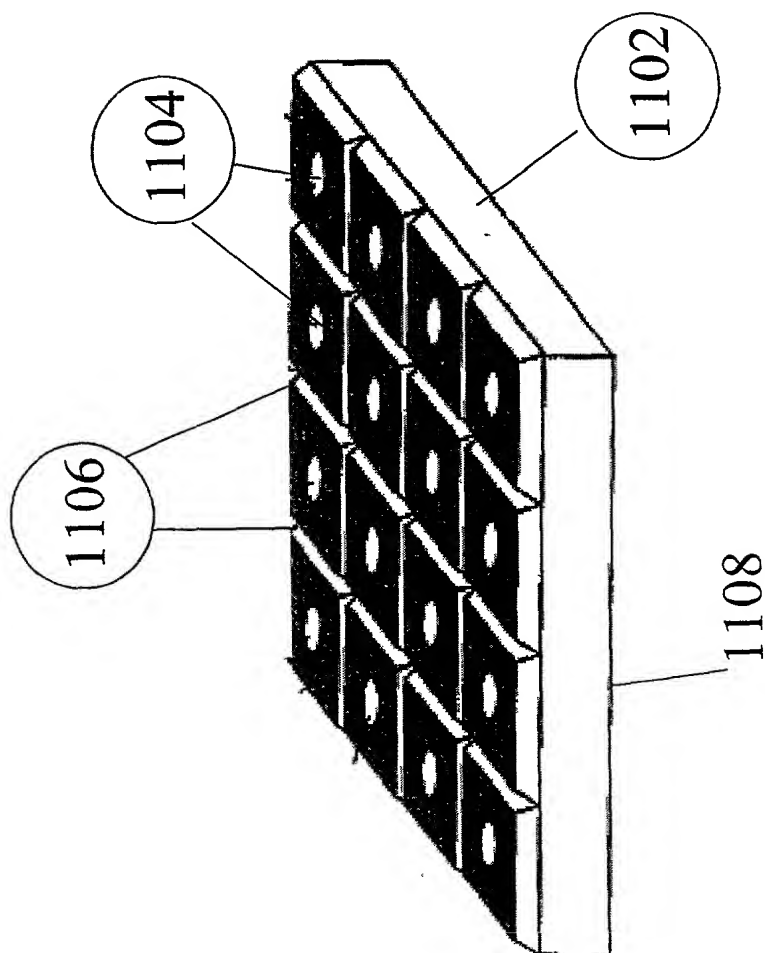


Figure 11

2046645

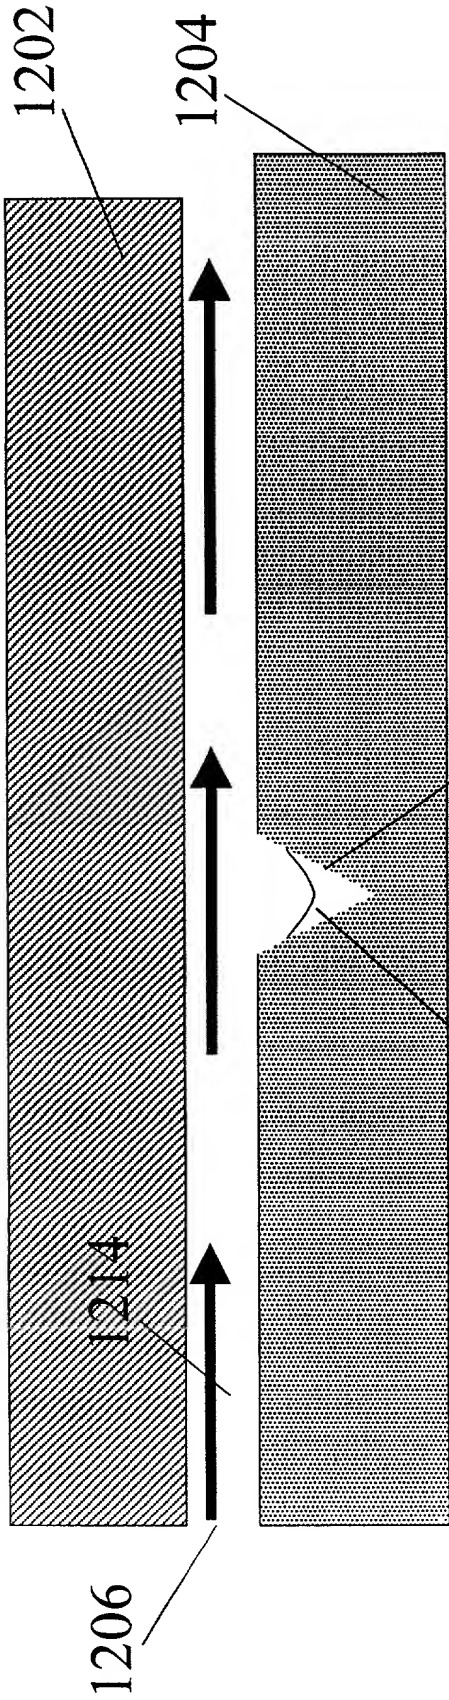


Figure 12A 1208 1210 1212

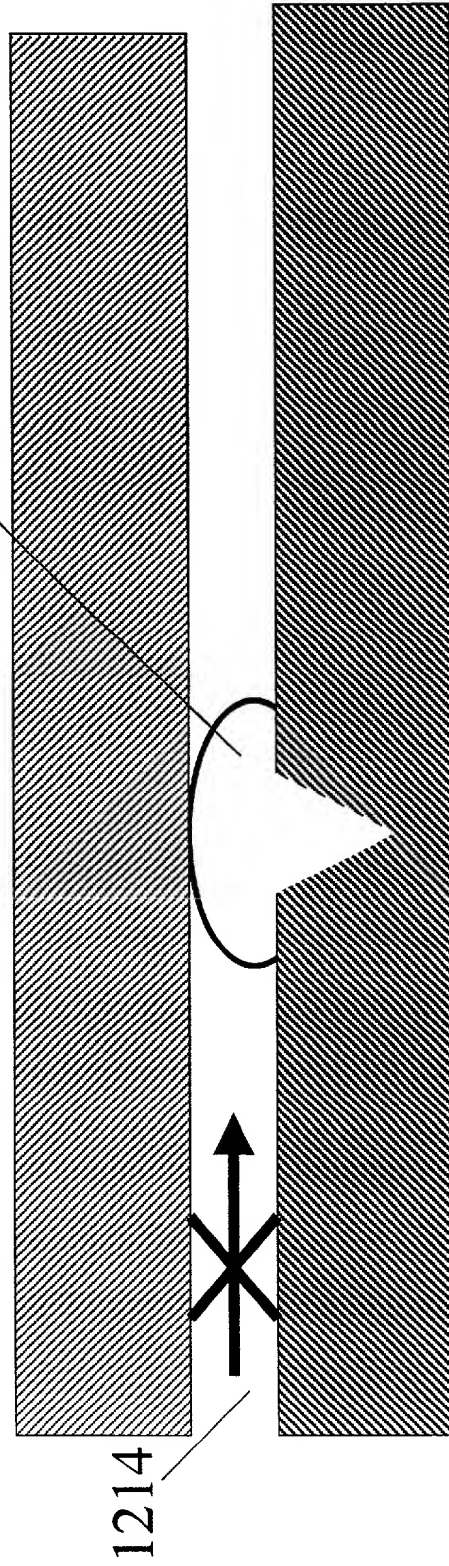
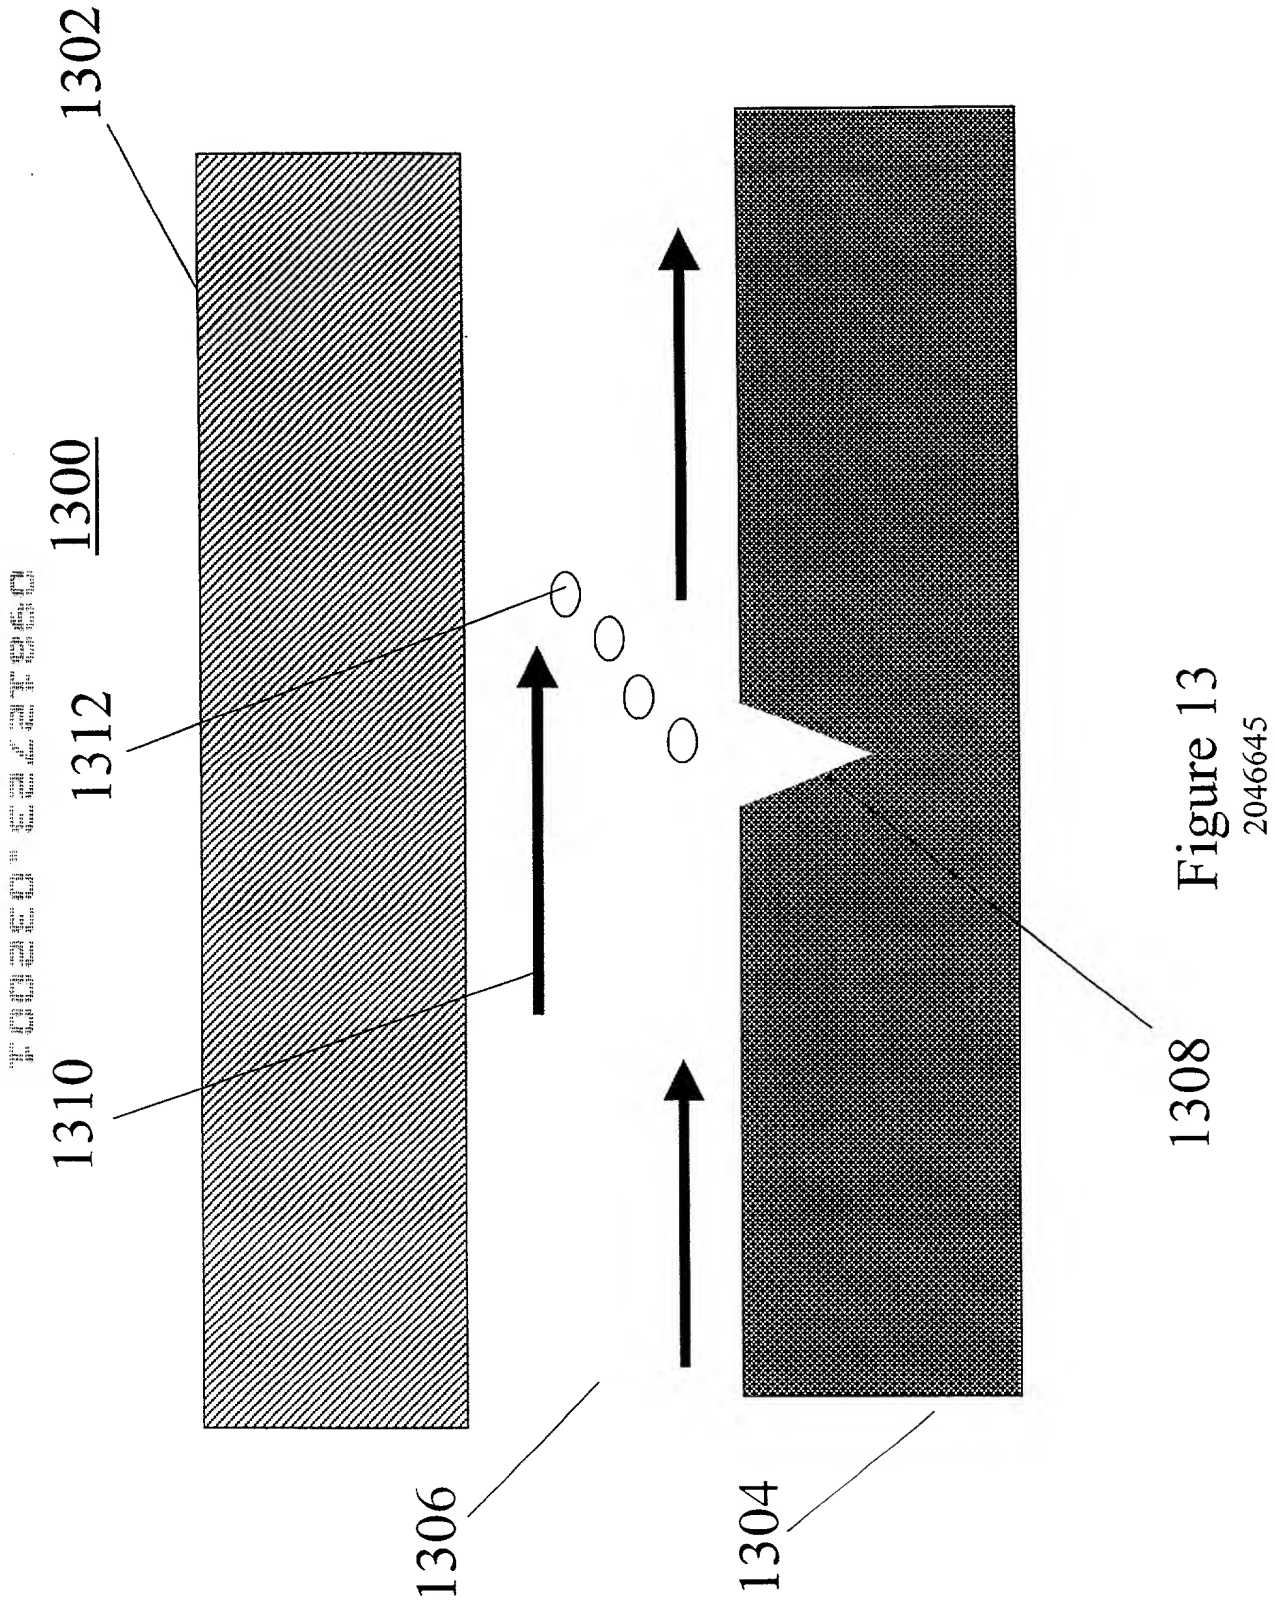


Figure 12B 2046645



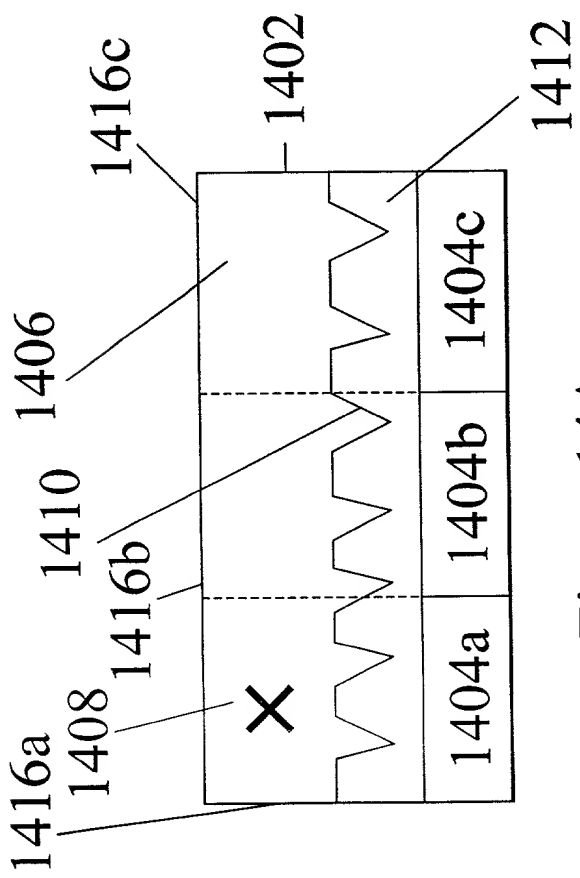


Figure 14A

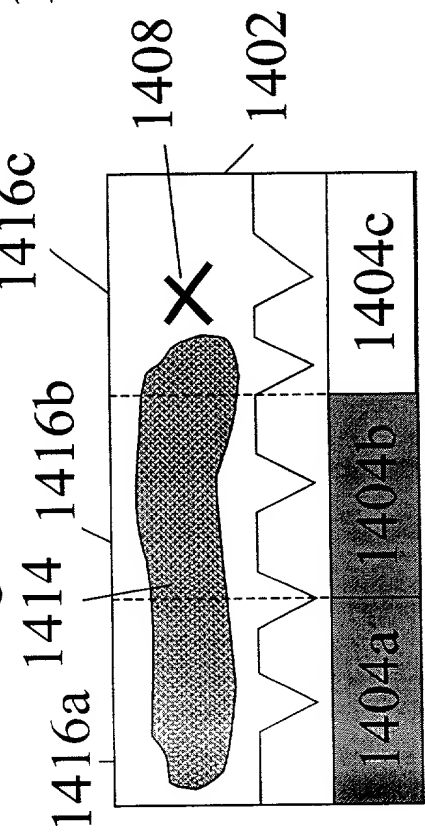


Figure 14B

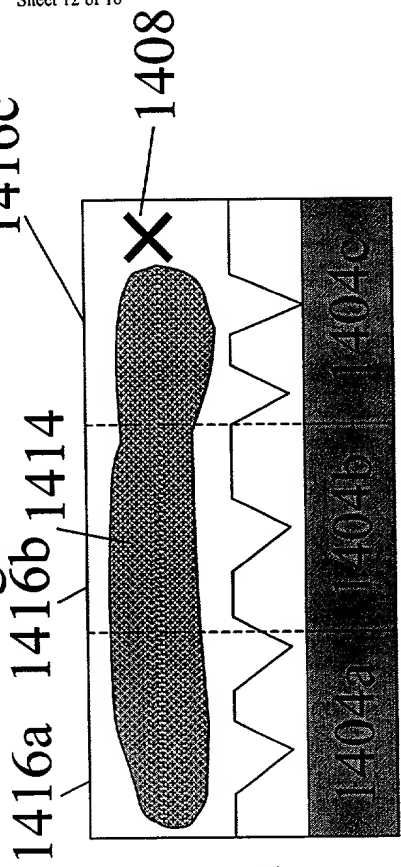
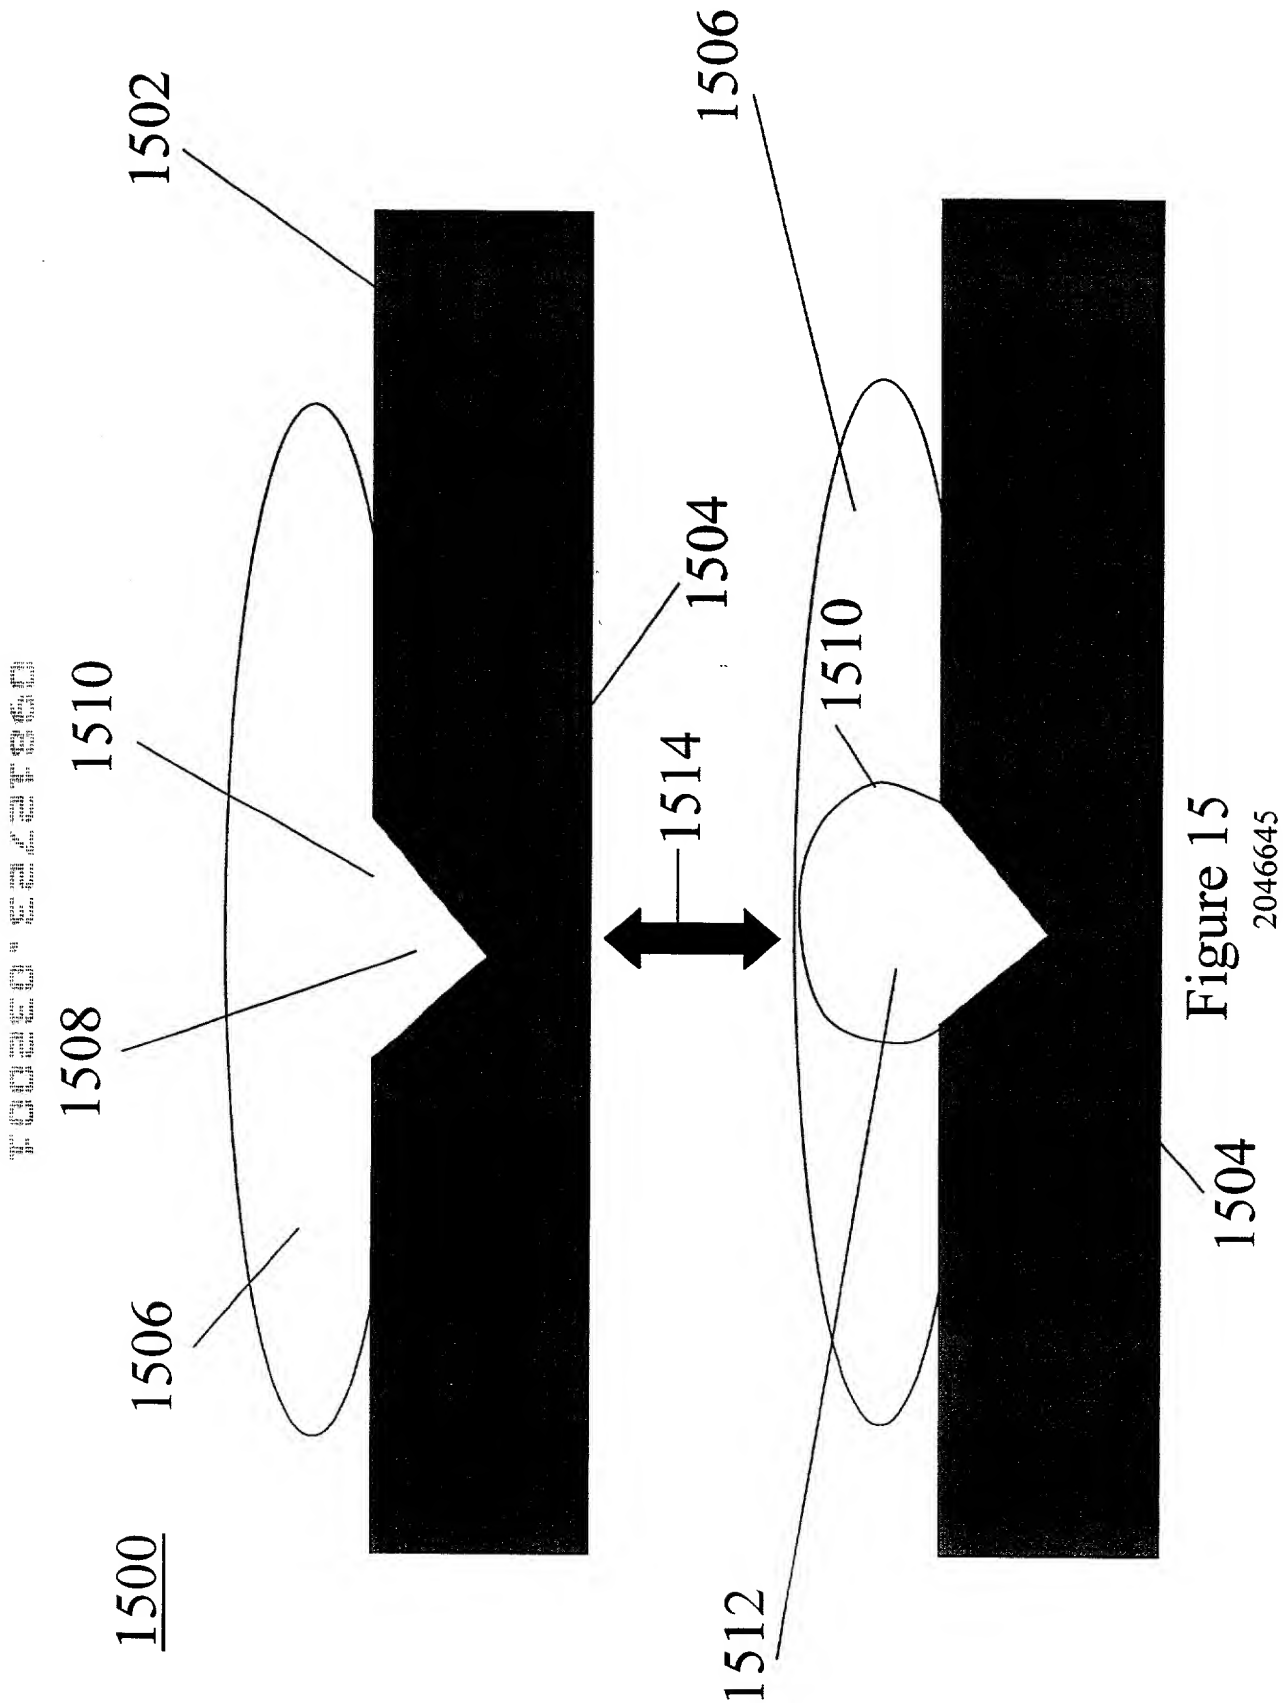


Figure 14C

Figure 14D

2046645



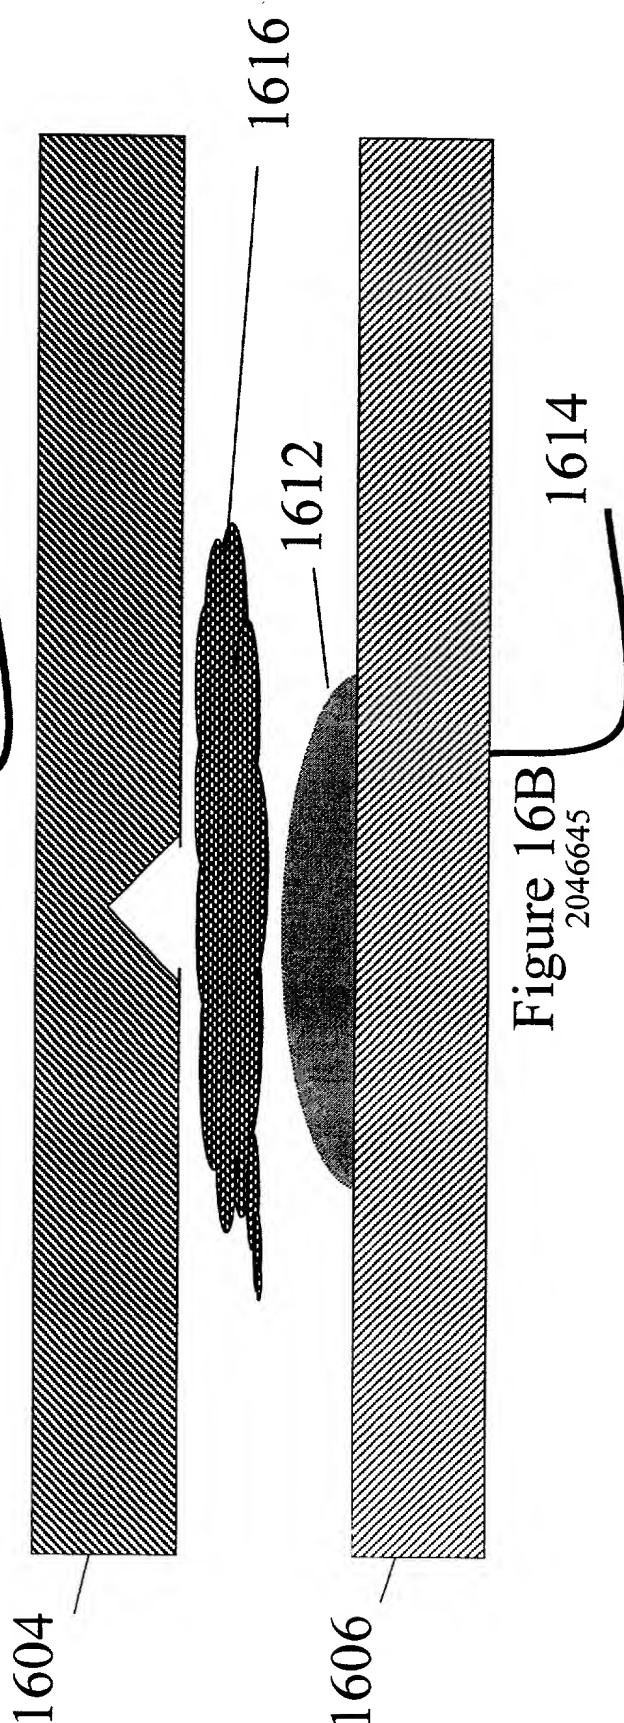
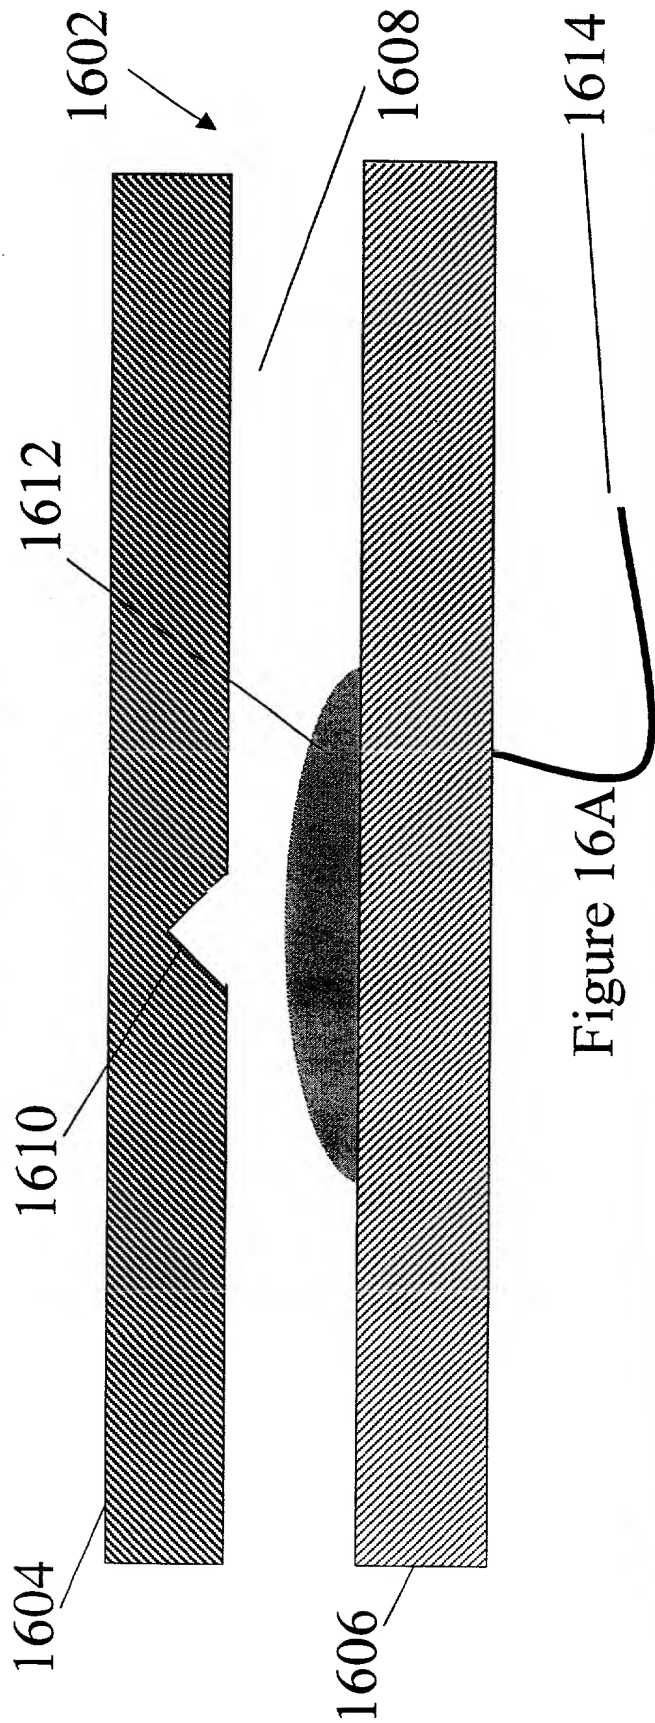


FIG. 17

1700

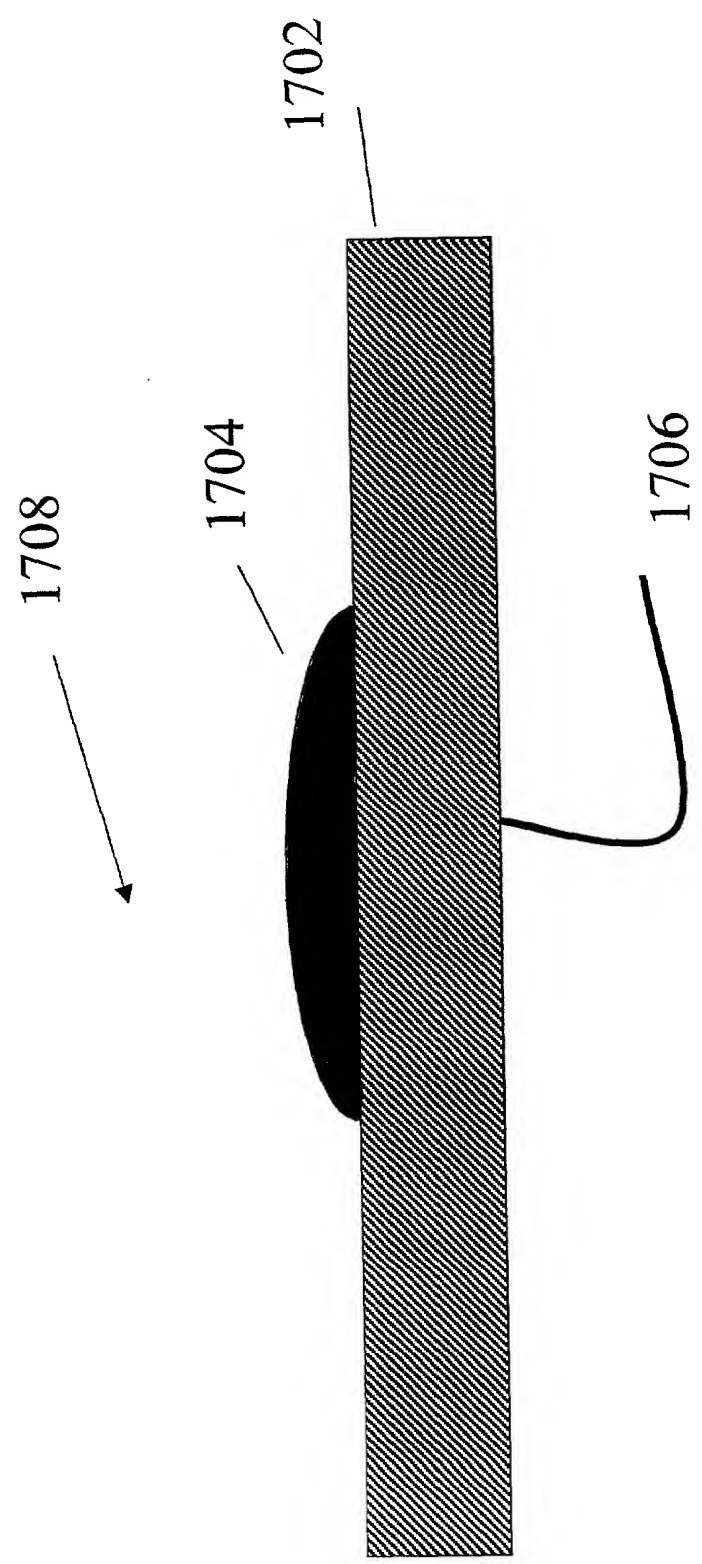


Figure 17

2046645

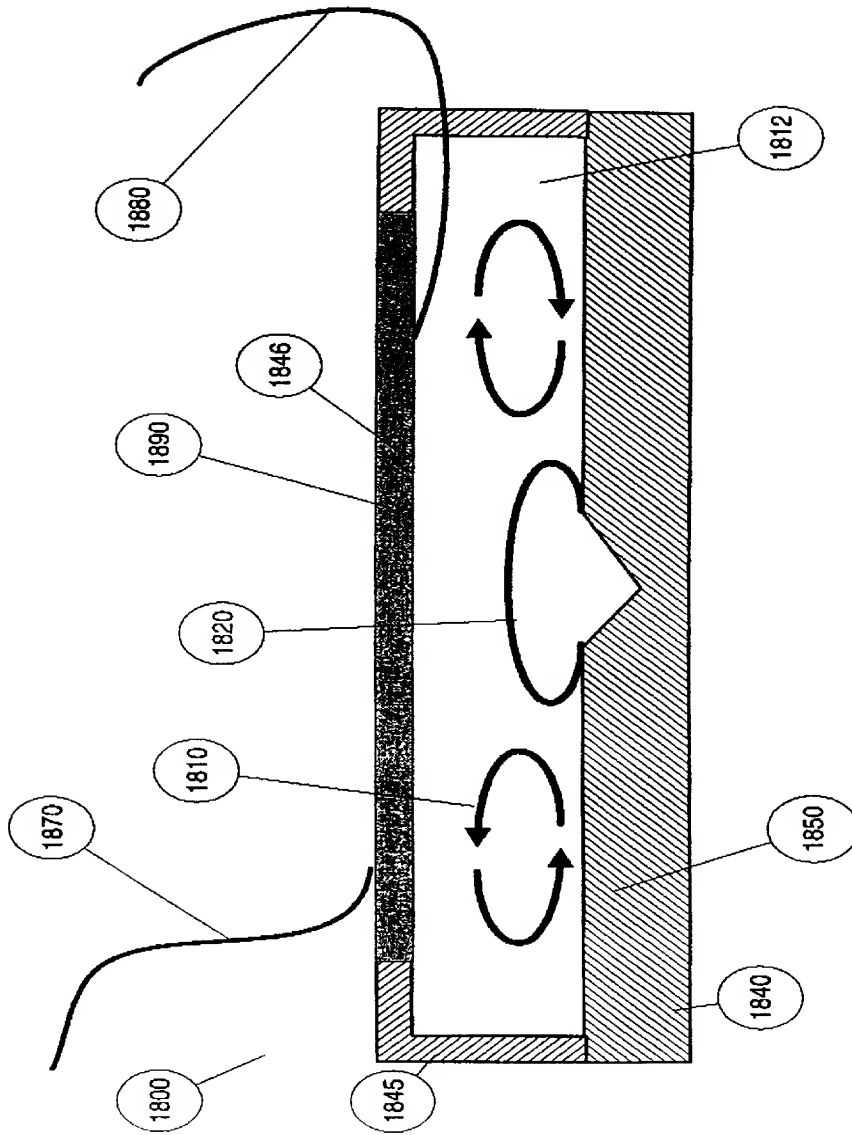


FIGURE EIGHTEEN